COPAL® knee moulds

FEMORAL COMPONENT

DIMENSIONS AND SPECIFICATIONS

	Anterior height	Posterior height	Distal thickness	M/L	Inner A/P	Outer A/P
	A	B	C	D	E	F
Size S	53	34.6	8.1	60	43	58
Size M	60.5	38.7	9.4	70	48	63
Size L	69	42.8	10.8	80	52	68

Measurements in mm; M/L = medial/lateral; A/P = anterior/posterior

FILLING VOLUME

Recommended number of packages of bone cement (1×40)		
Size S	Size M	Size L
1	2	2

Please note:
- Filling volume measured using the PALAMIX® vacuum mixing system and Heraeus bone cement. The volume of other bone cements may deviate from these figures and there may be different quantities of residual cement in other mixing systems.
- Additional bone cement for fixation of spacer might be required.

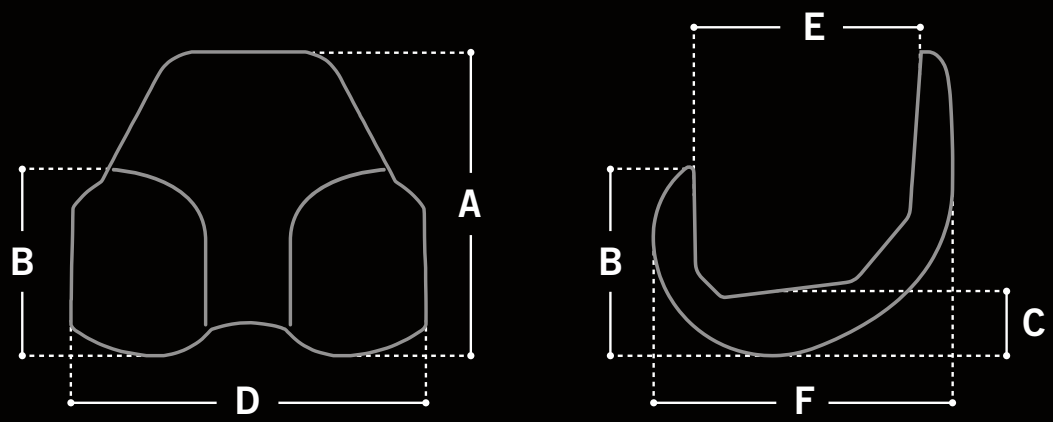

COPAL® knee moulds

TIBIAL COMPONENT

DIMENSIONS AND SPECIFICATIONS

	M/L	A/P	Stem length	Proximal stem	Distal stem
	G	H	I	J	K
Size S	65	45	30	20	11.3
Size M	75	49	30	20	11.3
Size L	85	53	30	20	11.3

Measurements in mm; M/L = medial/lateral; A/P = anterior/posterior

FILLING VOLUME

Recommended number of packages of bone cement (1×40)			
	Size S	Size M	Size L
12 mm	2	2	2
17 mm	2	2	2
22 mm	2	2	2
27 mm	2	2	3
32 mm	2	3	3
37 mm	3	3	3

Please note:
- Filling volume measured using the PALAMIX® vacuum mixing system and Heraeus bone cement. The volume of other bone cements may deviate from these figures and there may be different quantities of residual cement in other mixing systems.
- Additional bone cement for fixation of spacer might be required.

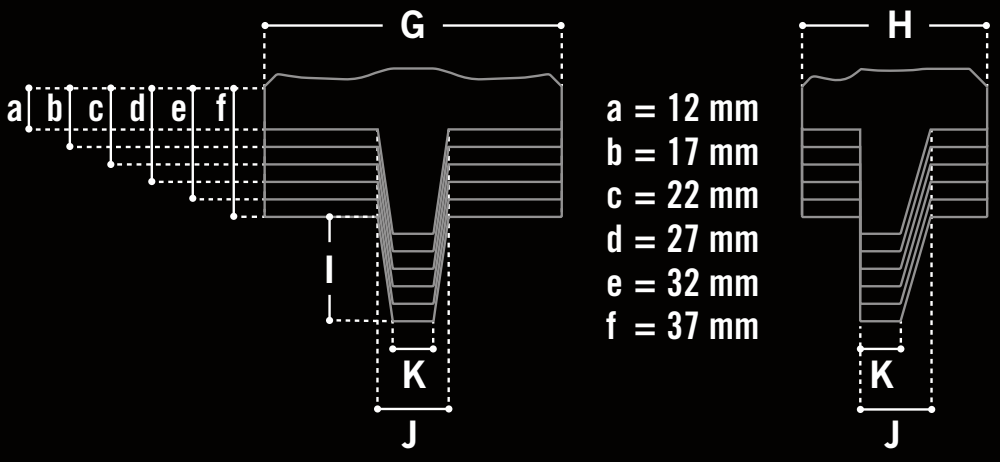

www.heraeus-medical.com

13033 INT